

AFRRI

93-4

TECHNICAL REPORT

Reference Dosimetry for the 1992 NATO Battlefield Dosimetry Intercomparison at the Army Pulse Radiation Facility



Leon J. Goodman
Betty A. Torres
James C. Myska
Brian Veit
Mark Oliver
Michael Stanka
Joel Dhermain
Bruno A. Asselineau

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE April 1993	3. REPORT TYPE AND DATES COVERED Technical Report	
4. TITLE AND SUBTITLE Reference Dosimetry for the 1992 NATO Battlefield Dosimetry Intercomparison at the Army Pulse Radiation Facility			5. FUNDING NUMBERS PE: NWED QAXM	
6. AUTHOR(S) Goodman, L.J., Torres, B.A., Myska, J.C., Veit, B., Oliver, M., Stanka, M., Dhermain, J., Asselineau, B.A.				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Armed Forces Radiobiology Research Institute 8901 Wisconsin Ave. Bethesda, Md. 20889-5603			8. PERFORMING ORGANIZATION REPORT NUMBER TR-93-4	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES) Defense Nuclear Agency 6801 Telegraph Road Alexandria, Va. 22310-3398			10. SPONSORING/MONITORING AGENCY REPORT NUMBER	
11. SUPPLEMENTARY NOTES				
12a. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution unlimited.			12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words)				
14. SUBJECT TERMS			15. NUMBER OF PAGES 14	
			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT UNCLASSIFIED	18. SECURITY CLASSIFICATION OF THIS PAGE UNCLASSIFIED	19. SECURITY CLASSIFICATION OF ABSTRACT UNCLASSIFIED	20. LIMITATION OF ABSTRACT SAR	

CLASSIFIED BY:

DECLASSIFY ON:

Reference Dosimetry for the 1992 NATO Battlefield Dosimetry Intercomparison at the Army Pulse Radiation Facility

**Leon J. Goodman⁽¹⁾, Betty A. Torres⁽¹⁾, James C. Myska⁽¹⁾,
CPT Brian Veit, USA⁽²⁾, Mark Oliver⁽²⁾, Michael Stanka⁽²⁾,
Joel Dhermain, Ph.D.⁽³⁾, Bruno A. Asselineau⁽³⁾**

⁽¹⁾Armed Forces Radiobiology Research Institute, Bethesda, Maryland.;

⁽²⁾Army Pulse Radiation Facility, Aberdeen Proving Ground, Maryland.;

⁽³⁾Etablissement Technique Central de l'Armement, Arcueil-Cedex, France

April 1993

Radiation Biophysics Department

ARMED FORCES RADIOBIOLOGY RESEARCH INSTITUTE

8901 Wisconsin Avenue
Bethesda, Maryland 20889-5603

Supported by the Armed Forces Radiobiology Research Institute, Defense Nuclear Agency. Views presented in this paper are those of the authors; no endorsement by the Defense Nuclear Agency has been given or should be inferred.

Contents

Introduction	1
Radiation Fields	1
Measurements	6
Results	7
Uncertainties	10
Comparison to Previous Data	11
Conclusion	12
Acknowledgement	12
References	13

Introduction

A NATO Dosimetry Study was performed from 23 March to 3 April 1992 at the Army Pulse Radiation Facility (APRF), Aberdeen Proving Grounds, Aberdeen, Maryland. This study was designed to determine the accuracy of battlefield dosimeters in a simulated tactical environment, and to compare the different NATO dosimeters in simple, well-defined radiation fields. Dosimeters were irradiated in four radiation fields: in free air (FIA) and on the surface of polyethylene phantoms by the APRF reactor with the core bare and with the core shielded by a converter shield.

Measurements to provide reference dosimetry for the NATO Dosimetry Study were made the week before and the week following the above dates and also during the second week of the battlefield dosimeter comparisons. Reference dosimetry for the NATO Dosimetry Study reactor irradiations was performed by three dosimetry groups.

1. Etablissement Technique Central de l'Armement (ETCA), Arcueil-Cedex, France
2. Armed Forces Radiobiology Research Institute (AFRRI), Bethesda, Maryland, USA
3. Army Pulse Radiation Facility (APRF), Aberdeen, Maryland, USA


Tissue kerma rates FIA and on the surface of phantoms, normalized to reactor power, were measured using paired ionization chambers, a neptunium fission chamber, diodes, rhodium foils, and aluminum oxide and calcium fluoride thermoluminescent dosimeters. For these measurements, the reactor was operated in the steady-state mode. Monitor sulfur pellets and calcium fluoride thermoluminescent dosimeters were used to establish tissue kerma in the pulsed environment used for the irradiation of the battlefield dosimeters.

This report contains a brief description of the radiation facilities and the measurements, and a comparison to the reference dosimetry data of the 1986 NATO battlefield dosimetry intercomparison.

Radiation Fields


The APRF "fast burst" reactor is a bare critical assembly that may be operated at power levels up to 10 kW and at super-prompt criticality to produce pulses with microsecond durations (1-3). For these studies, the reactor was operated inside the reactor silo with the center 2 m above the floor. All dosimetry measurements were made 1.65 m from

the core center and 2 m above the floor (see Figures 1 and 2). The converter shield, when used, was placed in front of the reactor core to better approximate the neutron spectrum 1 km down-range of a nuclear blast. The shield, 12.7 cm thick and 46 cm high, was constructed of polyethylene loaded with cadmium oxide (5% by weight).

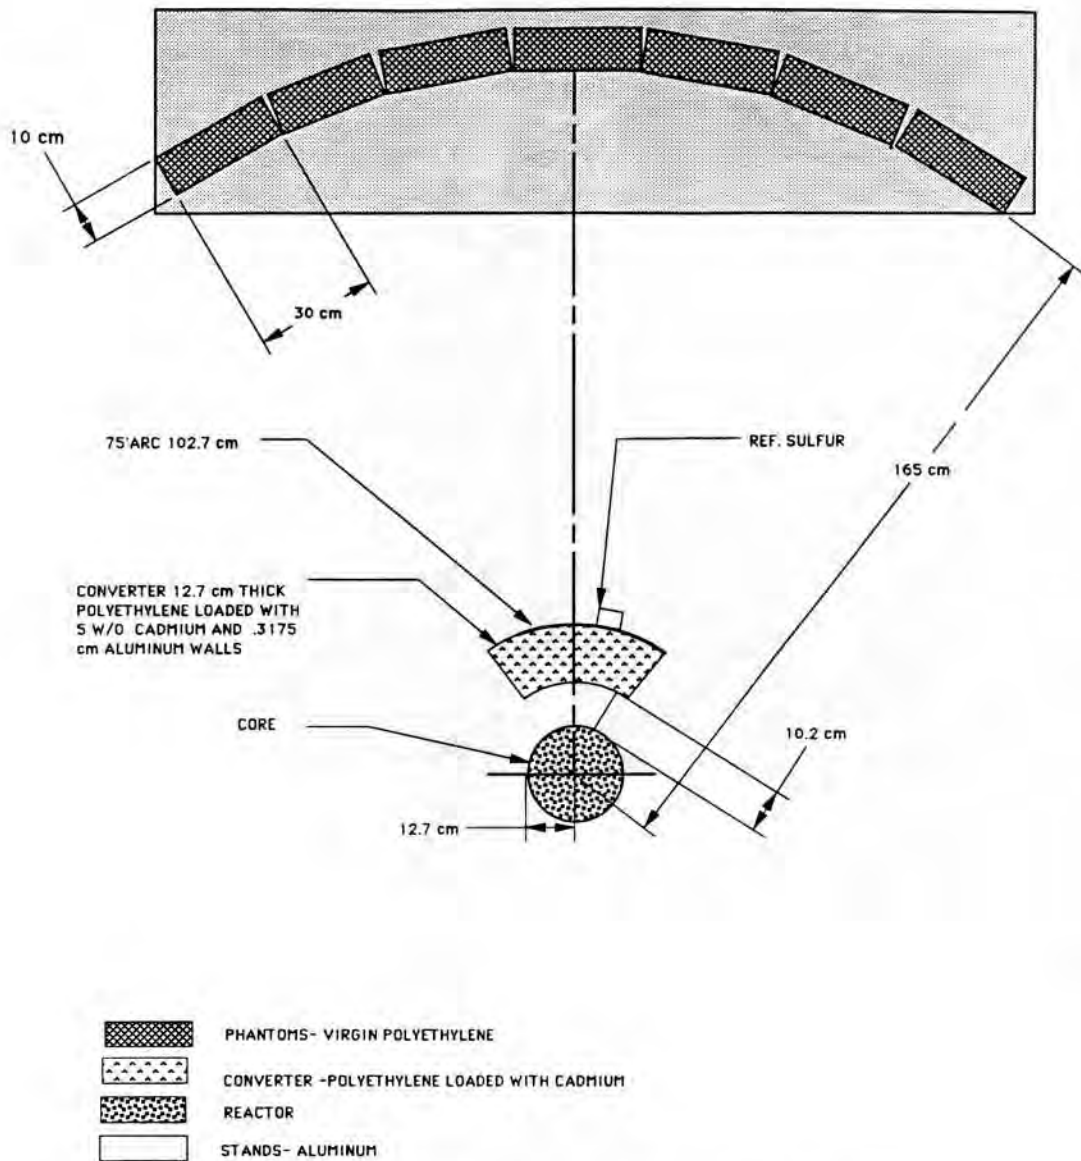

EXPOSURE CONFIGURATION WITH CONVERTER AND SLAB PHANTOMS -TOP VIEW

Figure 1. Top-view diagram of irradiation configuration showing the reactor core, the converter shield, and the polyethylene slab phantoms.

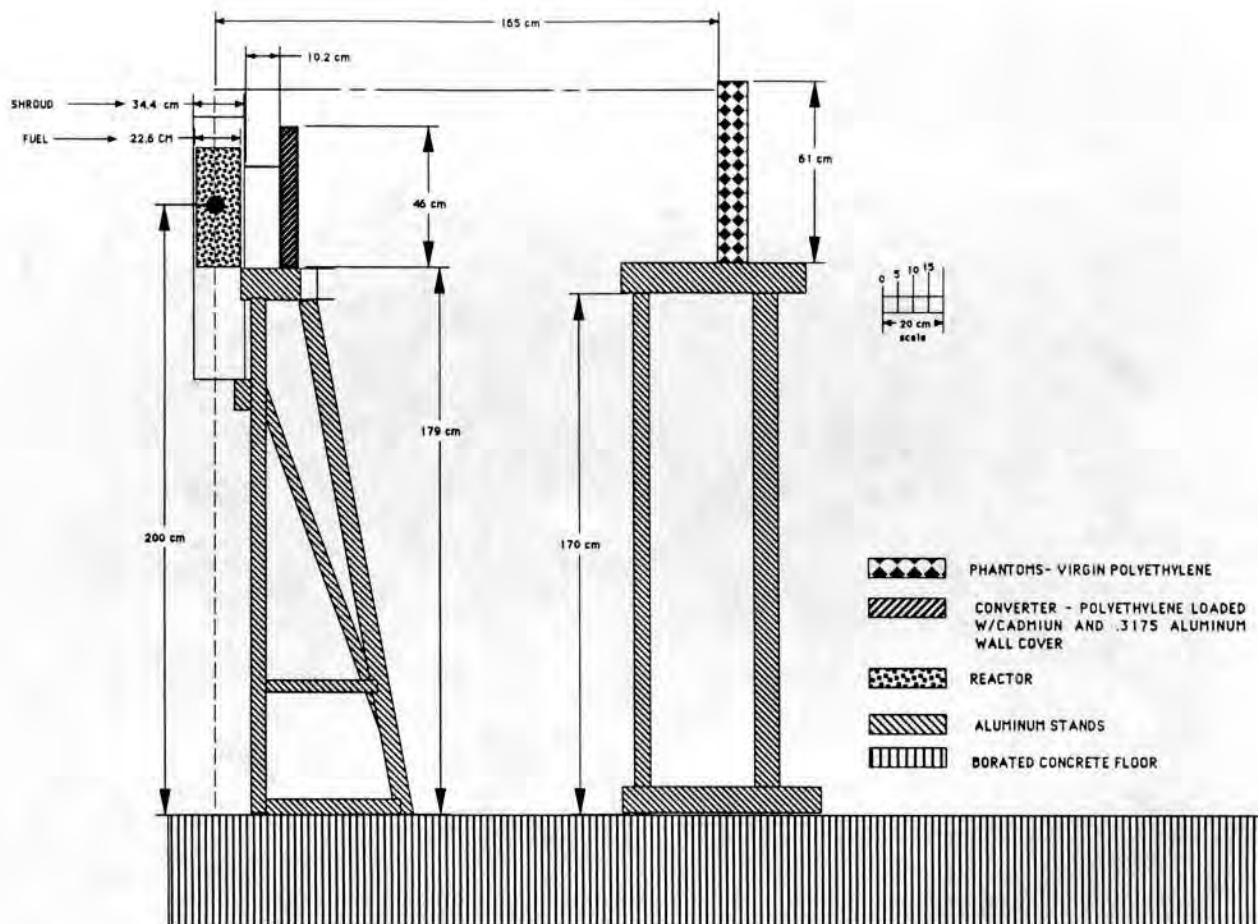

EXPOSURE CONFIGURATION WITH CONVERTER AND SLAB PHANTOMS- SIDE VIEW

Figure 2. Side-view diagram of irradiation configuration showing the reactor core with the converter shield and the polyethylene slab phantoms mounted on aluminum stands.

Spectral data for the unshielded APRF configuration were given in a previous technical report (4). Spectral data behind the converter shield are not available, but the qualitative effects of the shield were to reduce the neutron component of the tissue kerma in free air from 92% to 43%, and to produce a harder (more energetic) neutron spectrum. (Neutrons are absorbed by the hydrogenous material, decreasing the fast neutron flux and increasing the gamma-ray flux from hydrogen and cadmium capture reactions. Cadmium absorbs thermal and low-energy neutrons.)

For the irradiations made in free air, the dosimeters were mounted on a thin aluminum screen (see Figure 3) placed along a circular arc located at 1.65 m from the core centerline. When the phantoms were used, the screen was removed and the phantoms (polyethylene blocks 61 cm high, 30 cm wide, and 10 cm thick) were placed along this



Figure 3. Ionization chambers mounted on the aluminum screen for measurements in free air.

same arc (see Figure 1). The dosimeters were mounted directly on the front surface of the phantoms (see Figure 4). The aluminum screen, the phantoms, and the converter shield were supported by aluminum stands (see Figure 2).

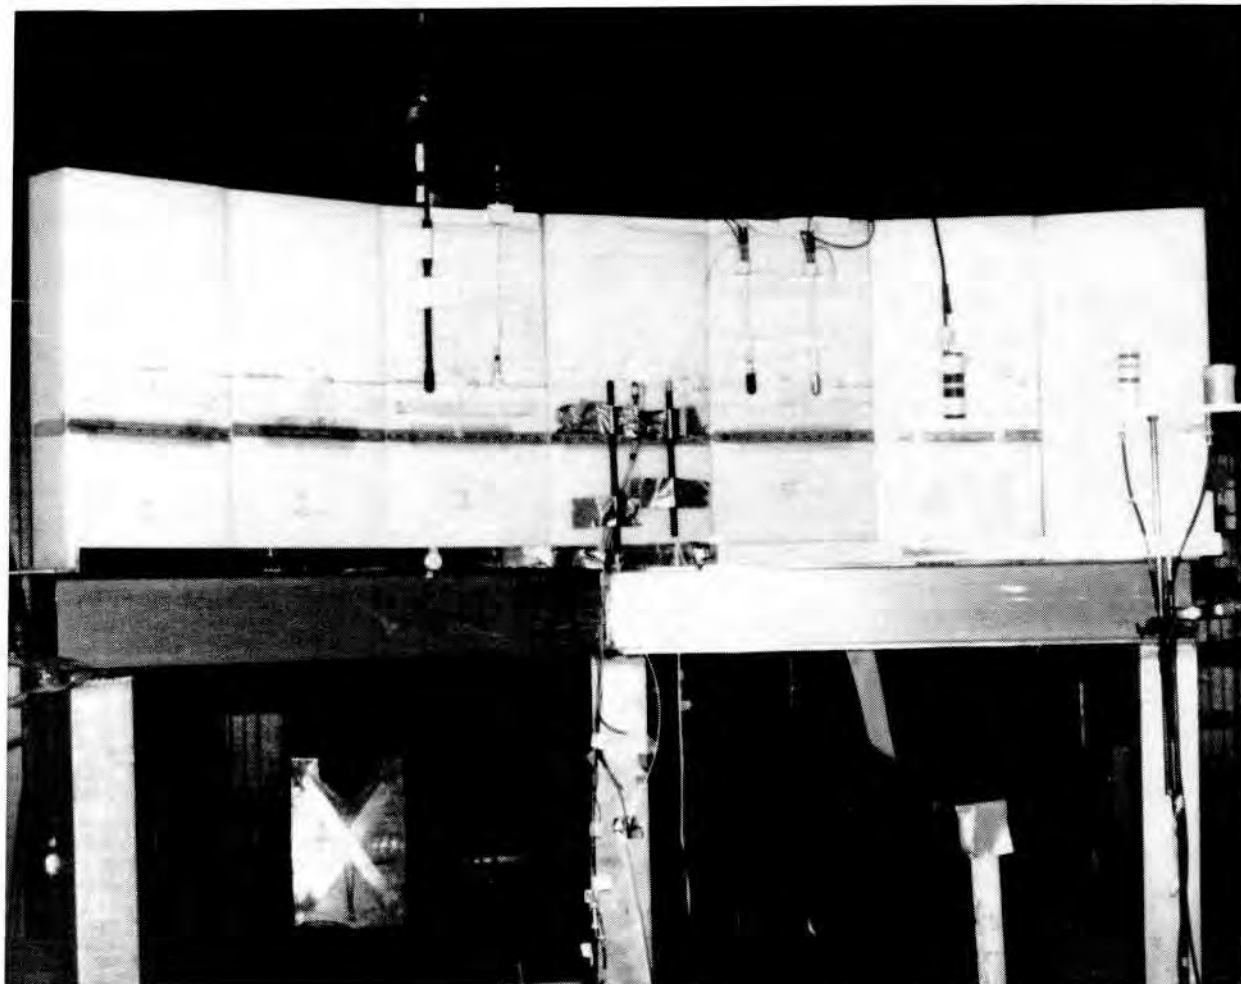


Figure 4. Ionization chambers, the fission chambers, and sulfur pellets mounted on the front surface of the polyethylene slab phantoms.

Measurements

The reactor reference dosimetry was performed with the reactor operated in the steady-state mode and was based on measurements made using a variety of dosimeters.

1. ETCA

- (a) Tissue-equivalent and magnesium-argon paired ionization chambers (TE-Mg IC)
- (b) Tissue-equivalent and aluminum-argon paired ionization chambers (TE-Al IC)
- (c) Tissue-equivalent and teflon-carbon dioxide paired ionization chambers (TE-C IC)
- (d) Neptunium fission chamber (Np FC)
- (e) Silicon diodes
- (f) Rhodium foils
- (g) Aluminum oxide thermoluminescent dosimeters (Al_2O_3 TLD)

2. AFRRI

- (a) Tissue-equivalent and magnesium-argon paired ionization chambers (TE-Mg IC)

3. APRF

- (a) Tissue-equivalent and magnesium-argon paired ionization chambers (TE-Mg IC)
- (b) Calcium fluoride thermoluminescent dosimeters (CaF TLD)

The measurement techniques applied for these dosimeters have been described in other reports (5-12). The measurement results obtained with these dosimeters were transferred to the pulsed environment through the use of sulfur monitor pellets and calcium fluoride TLDs.

Results

The results of the reference dosimetry measurements made in free air with the bare core are shown in Table 1. For this table and all subsequent tables the average total kerma and the average percent neutron kerma are calculated from the average neutron and gamma-ray kermas. The total kerma and percent neutron kerma calculated from the ionization chambers are presented for information. This configuration produced the radiation field with the largest component of neutron kerma, an average of 92%. It is notable that the variety of neutron dosimeters listed have a standard deviation (SD) of only 1%. The gamma-ray kermas, on the other hand, have a 13% SD, due mostly to a low (14.7) and a high (22.1) measurement. It is generally acknowledged that it is difficult to reliably measure a small gamma-ray component in a mixed neutron and gamma-ray field.

Table 1. Reference dosimetry measurements made in free air with a bare reactor core. All tissue kermas in mGy/(kW min). Note that the average total kerma and the average percent neutron kerma are calculated from the average neutron and gamma-ray kermas.

Group	Dosimeter type	Neutron kerma	Gamma-ray kerma	Total kerma	% neutron kerma
ETCA	TE-Mg IC	204	17.8	222	92
	TE-Al IC	204	17.3	221	92
	TE-C IC	207	14.7	222	93
	Np FC	204	--	--	--
	Diode	202	--	--	--
	Rh foil	203	--	--	--
	Al ₂ O ₃ TLD	--	17.0	--	--
AFRRI	TE-Mg IC	205	16.1	221	93
APRF	TE-Mg IC	205	17.6	223	92
	CaF TLD	--	22.1	--	--
	Average	204 +/- 1.5 (1%)	17.5 +/- 2.3 (13%)	222	92

Table 2 shows the results obtained when the dosimeters were mounted directly on the front surface of the phantoms and irradiated with the bare core. The effect of the phantoms is to increase by 5% the neutron kerma due to backscattering, and to increase the gamma-ray kerma by 2.6 times due to neutron-energy moderation and neutron capture by hydrogen in the phantoms. The net effect is to reduce the neutron kerma to 83% of the total kerma. For the larger component of gamma-rays now present, the measurements gave an SD=5%.

Table 2. Reference dosimetry measurements made on the surface of the phantoms with a bare reactor core. All tissue kermas in mGy/(kW min). Note that the average total kermas and average percent neutron kerma are calculated from the average neutron and gamma-ray kermas.

Group	Dosimeter type	Neutron kerma	Gamma-ray kerma	Total kerma	% neutron kerma
ETCA	TE-Mg IC	214	44.4	258	83
	TE-Al IC	212	46.5	258	82
	TE-C IC	210	47.5	258	82
	Np FC	217	--	--	--
AFRRI	TE-Mg IC	218	41.4	259	84
APRF	TE-Mg IC	215	45.1	260	83
	CaF TLD	--	46.8	--	--
	Average	214 +/- 3.0 (1%)	45.3 +/- 2.2 (5%)	259	83

The reference dosimetry measurements made in free air with the converter shield interposed between the core and the dosimeters are shown in Table 3. The introduction of this shield reduces the neutron kerma to only 18% of its former value and increases the gamma-ray kerma 2.7 times. The neutron kerma component is thus reduced to 43%. Even though fewer neutron dosimeters were used for these measurements, for the neutron kerma the SD is now increased to 6%. The gamma-ray kermas, however, now have SD=1%.

Table 3. Reference dosimetry measurements made in free air with the converter shield. All tissue kermas in mGy/(kW min). Note that the average total kerma and average percent neutron kerma are calculated from the average neutron and gamma-ray kermas.

Group	Dosimeter type	Neutron kerma	Gamma-ray kerma	Total kerma	% neutron kerma
ETCA	TE-Mg IC	35.1	46.7	81.8	43
	TE-Al IC	34.6	47.4	82.0	42
	TE-C IC	34.3	47.7	82.0	42
	Np FC	33.9	--	--	--
AFRRI	TE-Mg IC	36.9	47.5	84.4	44
APRF	TE-Mg IC	39.3	46.0	85.3	46
	CaF TLD	--	46.8	--	--
	Average	35.7 +/- 2.1 (6%)	47.0 +/- 0.6 (1%)	82.7	43

When measurements are made on the surface of the phantoms with the converter shield in place, the results shown in Table 4 are obtained. Compared to Table 3, there appears to be little effect due to neutron backscattering. The gamma-ray kerma, however, is 18% larger than the FIA measurements due to neutron-energy moderation and neutron capture by hydrogen. This configuration produces the lowest component of neutron kerma, 39%.

Table 4. Reference dosimetry measurements made on the surface of the phantoms with the converter shield. All tissue kermas in mGy/(kW min). Note that the average total kerma and the average percent neutron kerma are calculated from the average neutron and gamma-ray kermas.

Group	Dosimeter type	Neutron kerma	Gamma-ray kerma	Total kerma	% neutron kerma
ETCA	TE-Mg IC	35.8	55.6	91.4	39
	TE-Al IC	34.8	56.6	91.4	38
	TE-C IC	33.7	57.6	91.3	37
	Np FC	33.3	--	--	--
	Diode	33.0	--	--	--
	Al ₂ O ₃ TLD	--	52.0	--	--
AFRRI	TE-Mg IC	37.8	56.5	94.3	40
APRF	TE-Mg IC	39.0	56.4	95.4	41
	CaF TLD	--	52.4	--	--
	Average	35.3 +/- 2.3 (7%)	55.3 +/- 2.1 (4%)	90.6	39

Uncertainties

The precision of the ionization chamber measurements is generally better than 1%. The absolute accuracy of the paired ionization chamber method is considered to be around 5%-8%. When a component of the radiation field is small relative to the total kerma, however, the accuracy for determining this component may be considerably poorer.

The reference dosimetry measurements made in free air with the converter shield interposed between the core and the dosimeters are shown in Table 3. The introduction of this shield reduces the neutron kerma to only 18% of its former value and increases the gamma-ray kerma 2.7 times. The neutron kerma component is thus reduced to 43%. Even though fewer neutron dosimeters were used for these measurements, for the neutron kerma the SD is now increased to 6%. The gamma-ray kermas, however, now have SD=1%.

Table 3. Reference dosimetry measurements made in free air with the converter shield. All tissue kermas in mGy/(kW min). Note that the average total kerma and average percent neutron kerma are calculated from the average neutron and gamma-ray kermas.

Group	Dosimeter type	Neutron kerma	Gamma-ray kerma	Total kerma	% neutron kerma
ETCA	TE-Mg IC	35.1	46.7	81.8	43
	TE-Al IC	34.6	47.4	82.0	42
	TE-C IC	34.3	47.7	82.0	42
	Np FC	33.9	--	--	--
AFRRI	TE-Mg IC	36.9	47.5	84.4	44
APRF	TE-Mg IC	39.3	46.0	85.3	46
	CaF TLD	--	46.8	--	--
	Average	35.7 +/- 2.1 (6%)	47.0 +/- 0.6 (1%)	82.7	43

Manufacturer's specifications for the CaF TLDs gives a precision of $\pm 6.5\%$ for a group of 5000 chips. Measurements at APRF using 30 chips have verified this value. The CaF TLDs are calibrated with a Co-60 gamma-ray cell whose calibration is traceable to the National Institute of Standards and Technology. Groups of six TLDs are irradiated with doses ranging from 1 to 5000 Gy and the light output measured with a Harshaw 4000 reader is plotted versus dose to establish a calibration curve. Although the calibration of the gamma-ray cell is accurate to $\pm 3\%$, their accuracy for the reference dosimetry measurements depends on how well the calibrator spectrum compares to the gamma-ray spectrum produced by the reactor. Their accuracy for the gamma rays from the reactor is estimated to be $\pm 10\%$.

Measurements performed at AFRRI by J. H. Musk indicate a reproducibility within $\pm 4\%$ for Al_2O_3 TLDs (13).

Comparison to Previous Data

The results of the 1986 NATO reference dosimetry measurements were presented in a previous technical report (4). At that time, no measurements were made with the bare reactor core. Table 5 compares the 1986 ionization chamber results obtained using the converter shield with the 1992 (present) results for the configuration when the dosimeters were in free air. The difference between the two data sets is less than 2%.

Table 5. Comparison of 1986 and 1992 reference dosimetry for measurements made in free air using the converter shield. All tissue kermas in mGy/(kW min).

Data set	Neutron kerma	Gamma-ray kerma	Total kerma	% neutron kerma
1986	35.1	46.5	81.5	43
1992	35.7	47.0	82.7	43
1992/1986	1.017	1.011	1.015	--

When the dosimeters were mounted on the surface of the phantoms and the converter shield was used, the comparison of the 1986 and 1992 data sets is as shown in Table 6. It can be seen that the present data for neutron kerma are, on average, about 6% lower than the earlier data. Examination of Table 4 shows that this is due to the low values of neutron kerma obtained with the five ETCA dosimeters. The two values of neutron kerma obtained by the AFRRI and APRF ionization chambers are actually a little higher than the 1986 value. It is worth noting that ETCA did not participate in the 1986 reference dosimetry measurements.

Table 6. Comparison of 1986 and 1992 reference dosimetry for measurements made on the phantoms using the converter shield. All tissue kermas in mGy/(kW min).

Data set	Neutron kerma	Gamma-ray kerma	Total kerma	% neutron kerma
1986	37.6	54.9	92.5	41
1992	35.3	55.3	90.6	39
1992/1986	0.939	1.007	0.979	--

Conclusion

The reference dosimetry measurements described in this report serve to provide an absolute calibration of the tissue kerma rates in the radiation fields used for the 1992 NATO battlefield dosimeter intercomparison. Although a greater variety of dosimeters were used for these measurements than in the 1986 study, the eight dosimetry systems gave results which agreed well among themselves as well as with past values. Thus the kermas derived from these results can be used confidently to evaluate the accuracy of the NATO battlefield dosimeters intercompared in 1992.

Acknowledgement

The authors appreciate the help and cooperation provided by the APRF staff and thank them for helping to make this project a success.

References

1. Kazi, A. H. Operation of Army Pulsed Radiation Facility reactor core III. Transactions of American Nuclear Society 14: 313, 1971.
2. Kazi, A. H., Heimbach, C. R., Harrison, R. C., and Robitaille, H. A. Comparison of measured and calculated radiation transport in air-over-ground geometry to 1.6 km from a fission source. Nuclear Science and Engineering 85: 371-386, 1983.
3. Robitaille, H. A., and Hoffarth, B. E. A comparison of measured and calculated air-transported radiation from a fast, unshielded reactor. DREO Report No. 835, Defense Nuclear Establishment of Ottawa, Ottawa, 1980.
4. Dooley, M., Eagleson, D. M., Mohaupt, T. H., Kazi, A. H., and Zeman, G. H. Reference dosimetry for 1986 NATO battlefield dosimetry intercomparison at Army Pulsed Radiation Facility. Technical Report TR86-4, Armed Forces Radiobiology Research Institute, Bethesda, Maryland, 1986.
5. Goodman, L. J. A practical guide to ionization chamber dosimetry at the AFRRI reactor. Contract Report CR85-1, Armed Forces Radiobiology Research Institute, Bethesda, Maryland, 1985.
6. Neutron Dosimetry for Biology and Medicine. ICRU Report 26, International Commission on Radiation Units and Measurements, Bethesda, Maryland, 1977.
7. Broerse, J. J., Mijnheer, B. J., and Williams, J. R. European protocol for neutron dosimetry for external beam therapy. British Journal of Radiology 54: 882-898, 1981.
8. Waterman, F. M., Kuchnir, F. T., Skaggs, L. S., Kouzes, R. T., and Moore, W. H. Energy dependence of the neutron sensitivity of C-CO₂, MG-Ar, and TE-TE ionization chambers. Physics in Medicine and Biology 24: 721-733 1979.
9. Zeman, G. H., and Ferlic, K. P. Paired ion chamber constants for fission gamma-neutron fields. Technical report TR84-8, Armed Forces Radiobiology Research Institute, Bethesda, Maryland, 1984.
10. Ing, H., and Cross, W. G. A criticality neutron dosimeter using the Rh-103(n,n')Rh-103m reaction. Health Physics 25: 291-297, 1973.
11. Zeman, G. H. Rhodium-103 and indium-115 inelastic scattering reactions for fission neutron dosimetry. Technical Report TR84-7, Armed Forces Radiobiology Research Institute, Bethesda, Maryland, 1984.

12. Zeman, G. H., and Bice, W. S., Jr. Kerma factors for use in 37-group neutron spectrum calculations. Technical Report TR83-3, Armed Forces Radiobiology Research Institute, Bethesda, Maryland, 1983.
13. Musk, J. H., and Kearsley, E. Thermoluminescence characteristics of aluminum oxide. In: Programme and Abstracts, 10th International Conference on Solid State Dosimetry, p. 43. Nuclear Technology Publishing, Ashford, Kent, England, 1992.

DISTRIBUTION LIST

DEPARTMENT OF DEFENSE

ARMED FORCES INSTITUTE OF PATHOLOGY
ATTN: RADIOLOGIC PATHOLOGY DEPARTMENT

ARMED FORCES RADIOBIOLOGY RESEARCH INSTITUTE
ATTN: PUBLICATIONS DIVISION
ATTN: LIBRARY

ARMY/AIR FORCE JOINT MEDICAL LIBRARY
ATTN: DASG-AAFJML

ASSISTANT TO SECRETARY OF DEFENSE
ATTN: AE
ATTN: HA(IA)

DEFENSE NUCLEAR AGENCY
ATTN: TITL
ATTN: DDIR
ATTN: RARP
ATTN: MID

DEFENSE TECHNICAL INFORMATION CENTER
ATTN: DTIC-DDAC
ATTN: DTIC-FDAC

FIELD COMMAND DEFENSE NUCLEAR AGENCY
ATTN: FCFS

INTERSERVICE NUCLEAR WEAPONS SCHOOL
ATTN: TCHTS/RH

LAWRENCE LIVERMORE NATIONAL LABORATORY
ATTN: LIBRARY

UNDER SECRETARY OF DEFENSE (ACQUISITION)
ATTN: OUSD(A)/R&AT

UNIFORMED SERVICES UNIVERSITY OF THE HEALTH SCIENCES
ATTN: LIBRARY

DEPARTMENT OF THE ARMY

HARRY DIAMOND LABORATORIES
ATTN: SLCHD-NW
ATTN: SLCSM-SE

LETTERMAN ARMY INSTITUTE OF RESEARCH
ATTN: SGRD-ULY-OH

SURGEON GENERAL OF THE ARMY
ATTN: MEDDH-N

U.S. ARMY AEROMEDICAL RESEARCH LABORATORY
ATTN: SCIENTIFIC INFORMATION CENTER

U.S. ARMY ACADEMY OF HEALTH SCIENCES
ATTN: HSMC-FCM

U.S. ARMY CENTER FOR EW/RSTA
ATTN: AMSEL-RD-EW-SS

U.S. ARMY CHEMICAL RESEARCH, DEVELOPMENT, AND
ENGINEERING CENTER
ATTN: SMCCR-RST

U.S. ARMY INSTITUTE OF SURGICAL RESEARCH
ATTN: DIRECTOR OF RESEARCH

U.S. ARMY MEDICAL RESEARCH INSTITUTE OF CHEMICAL DEFENSE
ATTN: SGRD-UV-R

U.S. ARMY NUCLEAR AND CHEMICAL AGENCY
ATTN: MONA-NU

U.S. ARMY PULSE RADIATION FACILITY
ATTN: COMMANDER, USACSTA

U.S. ARMY RESEARCH INSTITUTE OF ENVIRONMENTAL MEDICINE
ATTN: SGRD-UE-RPP

U.S. ARMY RESEARCH OFFICE
ATTN: BIOLOGICAL SCIENCES PROGRAM

WALTER REED ARMY INSTITUTE OF RESEARCH
ATTN: DIVISION OF EXPERIMENTAL THERAPEUTICS

DEPARTMENT OF THE NAVY

NAVAL AEROSPACE MEDICAL RESEARCH LABORATORY
ATTN: COMMANDING OFFICER

NAVAL MEDICAL COMMAND
ATTN: MEDCOM-21

NAVAL MEDICAL RESEARCH AND DEVELOPMENT COMMAND
ATTN: CODE 40C

NAVAL MEDICAL RESEARCH INSTITUTE
ATTN: LIBRARY

NAVAL RESEARCH LABORATORY
ATTN: LIBRARY

OFFICE OF NAVAL RESEARCH
ATTN: BIOLOGICAL SCIENCES DIVISION

SURGEON GENERAL OF THE NAVY
ATTN: MEDICAL RESEARCH AND DEVELOPEMENT

DEPARTMENT OF THE AIR FORCE

BOLLING AIR FORCE BASE
ATTN: AFOSR

BROOKS AIR FORCE BASE
ATTN: AL/OEBSC
ATTN: USAFSAM/RZ
ATTN: AL/DEBL

NUCLEAR CRITERIA GROUP, SECRETARIAT
ATTN: OAS/XRS

SURGEON GENERAL OF THE AIR FORCE
ATTN: HQ USAF/SGPT
ATTN: HQ USAF/SGES

U.S. AIR FORCE ACADEMY
ATTN: HQ USAFA/DFBL

OTHER FEDERAL GOVERNMENT

ARGONNE NATIONAL LABORATORY
ATTN: BIOLOGY LIBRARY

BROOKHAVEN NATIONAL LABORATORY
ATTN: RESEARCH LIBRARY, REPORTS SECTION

CENTER FOR DEVICES AND RADIOLOGICAL HEALTH
ATTN: HFZ-110

DEPARTMENT OF ENERGY
ATTN: ER-72 GTN

GOVERNMENT PRINTING OFFICE
ATTN: DEPOSITORY RECEIVING SECTION
ATTN: CONSIGNED BRANCH

LIBRARY OF CONGRESS

ATTN: UNIT X

LOS ALAMOS NATIONAL LABORATORY

ATTN: REPORT LIBRARY/P364

NATIONAL AERONAUTICS AND SPACE ADMINISTRATION

ATTN: RADLAB

NATIONAL AERONAUTICS AND SPACE ADMINISTRATION, GODDARD
SPACE FLIGHT CENTER

ATTN: LIBRARY

NATIONAL CANCER INSTITUTE

ATTN: RADIATION RESEARCH PROGRAM

NATIONAL DEFENSE UNIVERSITY

ATTN: LIBRARY

NATIONAL LIBRARY OF MEDICINE

ATTN: OPI

U.S. ATOMIC ENERGY COMMISSION

ATTN: BETHESDA TECHNICAL LIBRARY

U.S. FOOD AND DRUG ADMINISTRATION

ATTN: WINCHESTER ENGINEERING AND
ANALYTICAL CENTER

U.S. NUCLEAR REGULATORY COMMISSION

ATTN: LIBRARY

RESEARCH AND OTHER ORGANIZATIONS

BRITISH LIBRARY (SERIAL ACQUISITIONS)

ATTN: DOCUMENT SUPPLY CENTRE

CENTRE DE RECHERCHES DU SERVICE DE SANTE DES ARMEES

ATTN: DIRECTOR

DEFENCE RESEARCH ESTABLISHMENT OTTAWA

ATTN: NUCLEAR EFFECTS SECTION

ETABLISSEMENT TECHNIQUE CENTRAL DE L'ARMEMENT

ATTN: CENTRE D'ETUDES DU BOUCHET

INHALATION TOXICOLOGY RESEARCH INSTITUTE

ATTN: LIBRARY

INSTITUTE OF NAVAL MEDICINE

ATTN: DEFENCE RADIOLOGICAL PROTECTION
SERVICE

INSTITUTE OF RADIOBIOLOGY

ARMED FORCES MEDICAL ACADEMY

ATTN: DIRECTOR

KAMAN SCIENCES CORPORATION

ATTN: DASIAC

NBC DEFENSE RESEARCH AND DEVELOPMENT CENTER OF THE
FEDERAL ARMED FORCES

ATTN: WWDBW ABC-SCHUTZ

MEDICAL BIOLOGICAL LABORATORY TNO

NCTR-ASSOCIATED UNIVERSITIES

ATTN: EXECUTIVE DIRECTOR

NORWEGIAN DEFENCE RESEARCH ESTABLISHMENT

ATTN: DIVISION FOR ENVIRONMENTAL
TOXICOLOGY

RUTGERS UNIVERSITY

ATTN: LIBRARY OF SCIENCE AND MEDICINE

UNIVERSITY OF CALIFORNIA

ATTN: LABORATORY FOR ENERGY-RELATED
HEALTH RESEARCH

ATTN: LAWRENCE BERKELEY LABORATORY

UNIVERSITY OF CINCINNATI

ATTN: UNIVERSITY HOSPITAL, RADIOISOTOPE
LABORATORY

WEHRWISSENSCHAFTLICHE DIENSTELLE

ATTN: NUCLEAR RADIATION EFFECTS

